

NovaSure® GEA refined

Provide an improved global endometrial ablation (GEA) experience with the enhanced **NovaSure ADVANCED device.**^{1*†}



ROUNDED TIPS
for easier insertion[†]

SMALLER DIAMETER
for approximately 6 mm of cervical dilation

IMPROVED CERVICAL SEAL
for an increased sealing surface²




NovaSure® ADVANCED

*A hysteroscopic study has shown that narrow instrument diameter correlates with less patient discomfort during the post-procedure recovery phase.
†Based on internal bench testing that measured perceived ease of insertion through a simulated cervix of both the 6-mm and 8-mm devices. N=16 surgeon users.


Refined... with patient and physician in mind

The next generation **NovaSure® ADVANCED** device is further refined to help you manage the GEA experience by providing more comfort for your patients.^{1*}

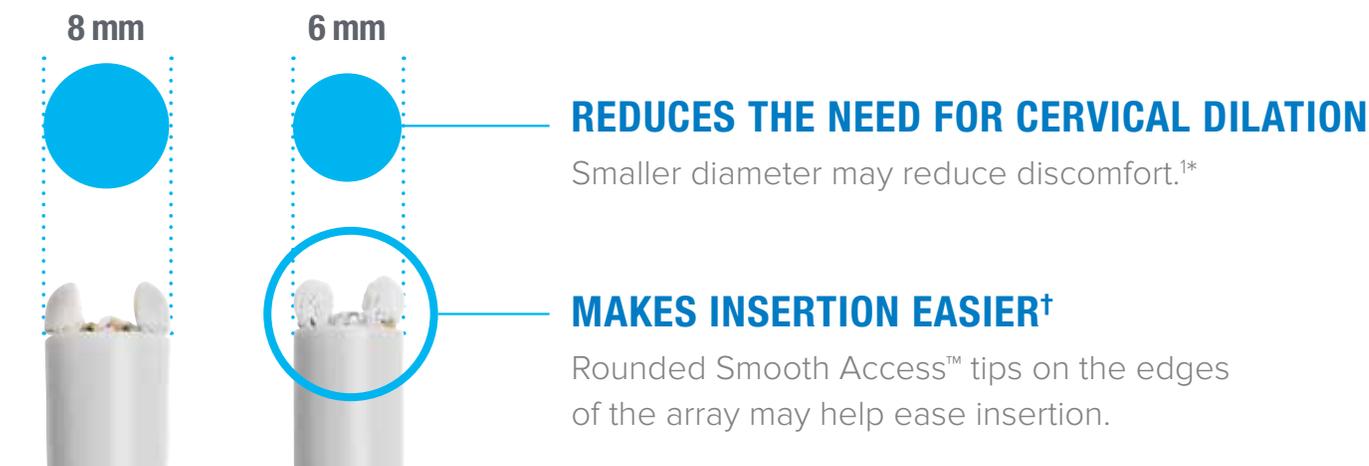

INCREASES SEALING SURFACE

Improved cervical seal creates an increased sealing surface within the cervical canal during proactive cavity integrity assessment and evacuation of procedure by-products.²



Manage challenging cases



The refined features may open opportunities to perform more procedures on women who have never been pregnant or who have had cesarean sections.

Abnormal uterine bleeding in a 40-year-old woman

- **Chief complaint:** menorrhagia for five years, causing symptomatic iron-deficiency anemia; has not responded to two treatments of hormonal therapy
- Pelvic exam reveals a nulliparous cervical os
- Confirmed: not interested in ever having children

*A hysteroscopic study has shown that narrow instrument diameter correlates with less patient discomfort during the post-procedure recovery phase.

†Based on internal bench testing that measured perceived ease of insertion through a simulated cervix of both the 6-mm and 8-mm devices. N=16 surgeon users.

Outpatient opportunities

The **NovaSure® ADVANCED** device may also allow you to perform more GEA procedures in-office. **Compared to women in hospital settings, women undergoing outpatient endometrial ablation^{3*}:**



EXPERIENCE LESS NAUSEA AND VOMITING



SPEND LESS TIME IN RECOVERY



REQUIRE LESS POSTOPERATIVE MEDICATION

Women undergoing outpatient procedures under a local anesthetic require significantly less time off from work and experience reduced loss of income.⁴

PATIENT REQUEST:

“Can the procedure be done in an outpatient setting? I’d like to minimize time away from home and work.”



*Based on a study of women (N=73) who underwent GEA in a hospital (n=34) versus in an outpatient setting (n=39).

Refined... for expanding your practice


The NovaSure® ADVANCED device means more opportunity for:



IMPROVING
PATIENT COMFORT^{1*}



PROVIDING GEA FOR
PATIENTS WITH NARROW
CERVICAL OSTIA



PERFORMING
MORE IN-OFFICE
PROCEDURES

Contact a sales representative or visit NovaSure.com/ADVANCED to learn more.

ORDERING INFORMATION

| CATALOG NUMBER | PRODUCT DESCRIPTION | QUANTITY | UNIT OF MEASURE |
|----------------|---|----------|-----------------|
| NS2013US | NovaSure ADVANCED device | 3 | Box |
| NS2013KITUS | Kit NovaSure ADVANCED device and SureSound®+ device | 3 | Box |
| RFC2010-115 | RF10 touchscreen controller | 1 | Ea |

IMPORTANT SAFETY INFORMATION

NovaSure® endometrial ablation is for premenopausal women with heavy periods due to benign causes who are finished childbearing. Pregnancy following the NovaSure procedure can be dangerous. The NovaSure procedure is not for those who have or suspect uterine cancer; have an active genital, urinary or pelvic infection; or an IUD. NovaSure endometrial ablation is not a sterilization procedure. Rare but serious risks include, but are not limited to, thermal injury, perforation and infection. Temporary side effects may include cramping, nausea, vomiting, discharge and spotting. Inform patients to contact you if they experience a possible side effect related to use of this product. For detailed benefit and risk information, please consult the IFU.

*A hysteroscopic study has shown that narrow instrument diameter correlates with less patient discomfort during the post-procedure recovery phase.

REFERENCES: 1. Pluchino N, Ninni F, Angioni S, et al. Office vaginoscopic hysteroscopy in infertile women: effects of gynecologist experience, instrument size, and distention medium on patient discomfort. *J Minim Invasive Gynecol.* 2010;17(3):344-350. 2. Hologic, Inc. Data on file;2016. 3. Marsh F, Thewlis J, Duffy S. Randomized controlled trial comparing Thermachoice III* in the outpatient versus daycase setting. *Fertil Steril.* 2007;87(3):642-650. 4. Kumar V, Chodankar R, Gupta JK. Endometrial ablation for heavy menstrual bleeding. *Womens Health (Lond).* 2016;12(1):45-52.

Licensed material is being used for illustrative purposes only. Any person depicted in the licensed material is a model.

MISC-04395-001 Rev. 001 ©2017 Hologic, Inc. Hologic, NovaSure, Smooth Access, SureSound, The Science of Sure, and associated logos are trademarks or registered trademarks of Hologic, Inc. and/or its subsidiaries in the United States and/or other countries.

NovaSure® ADVANCED